


ELIMINATE INTERLOCKING WITH THE QUICK UP METHOD



Quick Up®

TISSUE COLORED IMPLANT PICK-UP SYSTEM

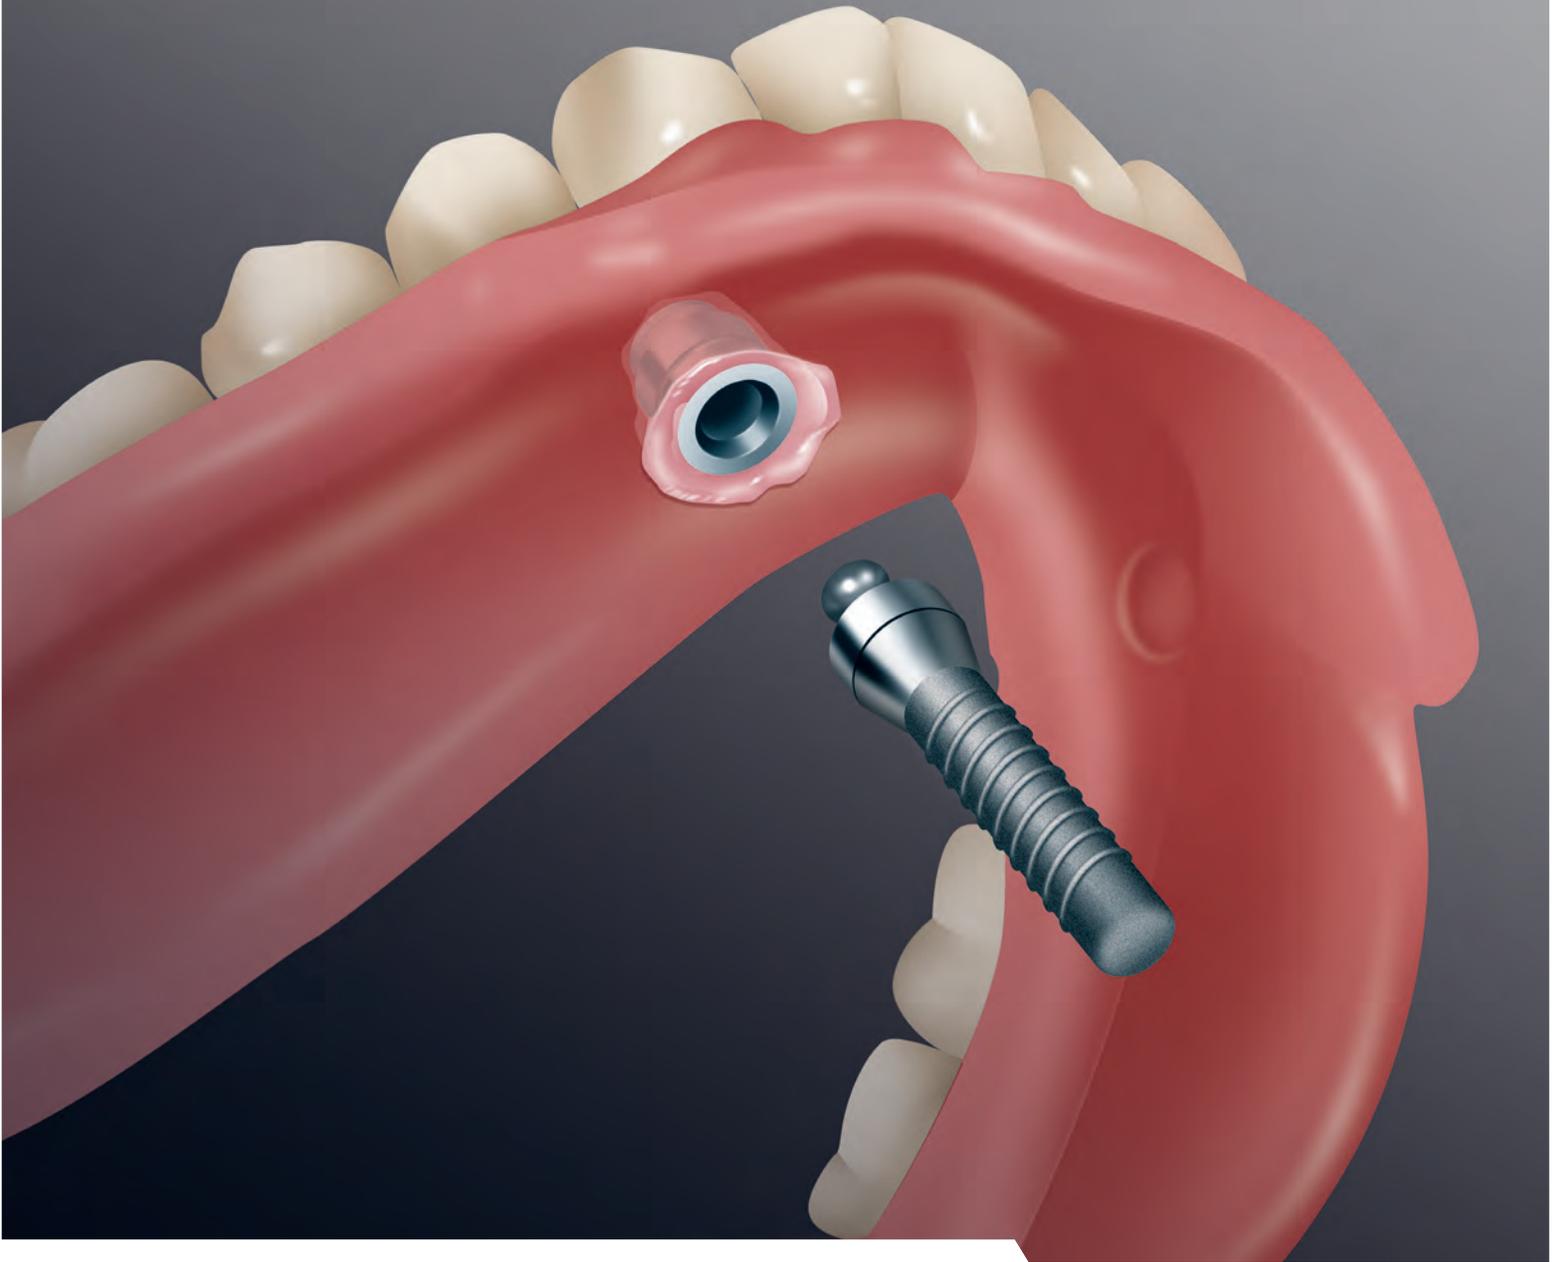

Quick Up®

THE NEW “QUICK UP” TECHNIQUE IN A COMPLETE SYSTEM THAT ELIMINATES THE RISK OF INTERLOCKING

Dentures are commonly used to replace missing teeth, however there can be difficulty in finding a proper fit due to bone atrophy, resorption processes, changes to the denture base which is made up of both hard and soft tissue.

To improve the fit and stability of dentures, implanting small diameter attachments into existing dentures is becoming an increasingly popular option. Dentists can simply attach secondary components to the existing denture, making a removable connection with the implants and thus offering patients greater comfort, convenience and affordability while saving themselves time and expense.

The Quick Up Kit contains all the components required for attaching female parts, attachments and other attachment elements to composite-based dentures. This means that Quick Up is also indicated for the reattachment of secondary components in dentures.

In developing Quick Up we attached great importance to making the product as easy-to-use as possible, so that the bonding of secondary components would be stress-free procedure for both the dentist and their patients, all while delivering predictable results. The steps for bonding secondary components always follow the same procedure: A relief must be immediately made around the implants after placement to facilitate irritation-free healing. In the next step the secondary components (female parts, attachments) must be attached to the denture base after the implants have healed (or immediately after placement in the case of immediate loading).

This procedure must be carried out on the patient to ensure a more accurate fit and requires that a check be made before the final intraoral bonding of the denture. Any corrections necessary can still easily be made. Moreover, the patient is spared the inconvenience of having to manage without a denture. This procedure saves the dentist a lot of time.

The marked areas are hollowed out to a large extent as preparation for bonding the secondary components into the denture base. This is done so that the denture can be inserted without any difficulty over the implants / root post caps with the secondary components attached. The dentist checks that the secondary components are securely seated into the denture base as well as carrying out the clinical check with Fit Test C & B, a special control and covering silicone.

The purpose of these checks is to enable the dentist to make any corrections required prior to using Quick Up and the final bonding stage without being pressed for time.

The additional application steps comprise simply removing Fit Test C & B from the denture base and if necessary, blocking out or covering the implants or primary components / male parts and the gingiva with Fit Test C & B in the patient's mouth.

The special adhesive is then applied to the denture base. The previously roughened secondary components / attachments are fitted in the patient's mouth and the holes in the denture base provided for the attachments are only filled approx. 2 / 3 full with Quick Up.

The denture is inserted and brought into occlusion under the supervision of the dentist.

Quick Up cures in just 3.5 minutes from the start of mixing. The denture can then be removed from the patient's mouth. The attachments or secondary components / female parts have now already been bonded into the denture base. Ditched areas are now quickly and systematically filled with the light-curing Quick Up LC. This procedure comprises the application of both self-curing Quick Up Material followed by correction with light-curing Quick Up LC. This is the best way of preventing a disastrous locking on of primary and secondary components. Finishing, polishing and the removal of the control silicone Fit Test C & B used for blocking out concludes the clinical procedure.

Quick Up®

BONDING OF ATTACHMENTS IN JUST THREE STEPS

First step:

- Mark the position of the secondary components on the denture base
- Determine the space required and check the secondary components




Quick Up®

QUICK UP® ADHESIVE PROVIDES A SECURE HOLD TO THE DENTURE

Second step:

- Wet prepared holes in the denture base with adhesive
- Place attachments / secondary components on the primary components in the mouth
- Cover areas to be protected, such as the gingiva and joint required, with the enclosed control and covering silicone Fit Test C & B
- Bond in the prepared secondary components in the denture base with Quick Up

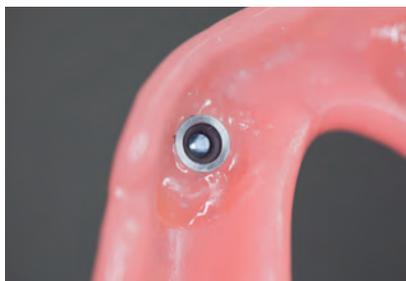


Quick Up®

CORRECTIONS EASILY MADE WITH QUICK UP® LC

Third step:

- Fill voids with Quick Up LC, if necessary
- Finishing and polishing

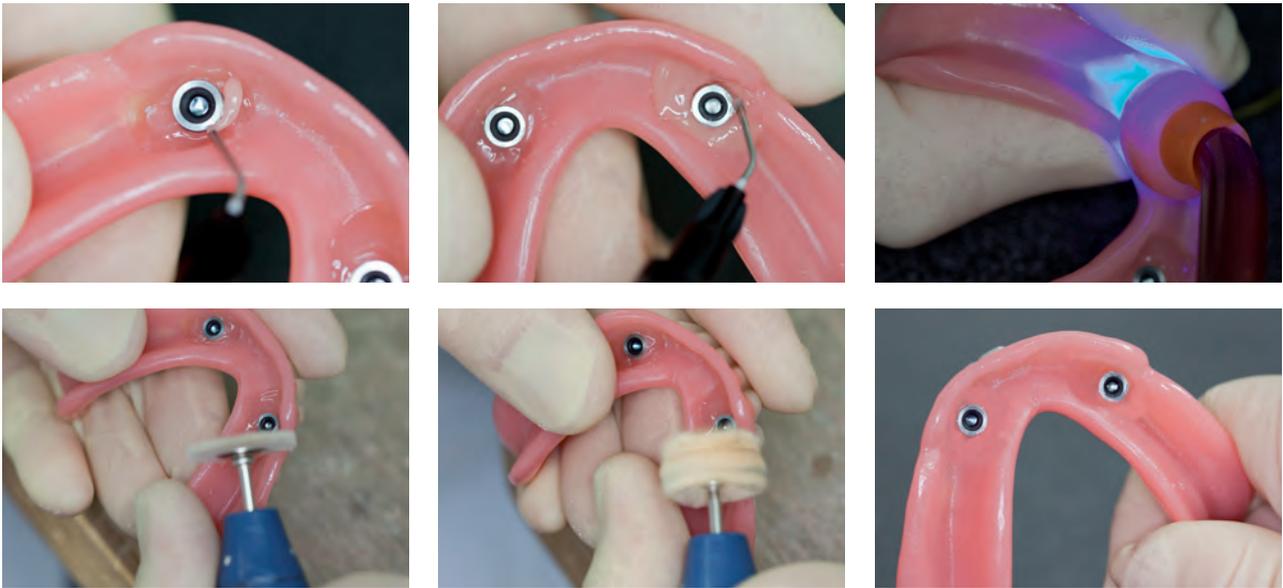

Quick Up® – the better alternative

Quick Up enables attachments and secondary components to be bonded into the patient's denture quickly and easily. Alternative systems that use soft relining materials instead of metal attachments for anchoring don't reach a comparable level of stability and suffer from numerous and frequent adjustments. Difficulties with mechanical or adhesive retention as well as a shorter material life span with soft relining materials are the reason for this.

In contrast, the cementation of metal attachments with Quick Up offers a solid solution with higher stability and less need for control and adjustments.

What users are saying

Dentists who already use Quick Up for Locator® systems and attachments were very positive about the composition of the kit and the individual components. This is what they had to say:

- “Very good handling thanks the small application syringe (especially intraorally)”
- “The shade was almost identical to acrylic resin”
- “Low material consumption”
- “A very simply designed product”

A dentist and lecturer from the US similarly wrote:

“Many thanks for the opportunity of using Quick Up. My experiences with this material have so far been extremely positive. I am impressed by the adhesive and the form of application, as well as by the light-curing correction material which is ideal for small ditched areas.”

Quick Up®

A SAFER, QUICKER AND MORE COST EFFECTIVE WAY TO DO YOUR IMPLANT PICK-UPS!

Indications

- The gingival-colored self-curing SC material is used for cementing attachments, such as ball, Locator® and telescopic anchors as well as other anchors in acrylic-based dentures
- The gingival-colored light-curing LC material can be used for subsequent corrections

Advantages

- Faster with Quick Up method: Work without vent holes and excess material removal; Underfill with 3.5 min. fast setting, self-cured material; finish with light-cured component
- Direct pick up results in more accuracy compared to indirect method
- Complete system with checking and block out silicone – Fit Test C & B
- Low heat, self-curing material avoids tissue irritations
- Tasteless and odorless
- High bond strength to acrylic denture base
- Allows pick up of any attachment

Optimized work flow improves the bottom line

The new Quick up method not only improves the clinical success rate, but also optimizes the work flow. In difficult economic times it becomes more and more important for clinicians to optimize work flows without compromising quality. The Quick Up method is a great example how a product can not only improve results, but furthermore improves the work flow and saves time and therefore money. Compared to indirect lab-processed bonding of denture housings, the clinician saves impression material, disinfection, chairside time and lab fees. But even if the direct pick up method is chosen there are differences. The new Quick Up method cut the procedure time in half and can save the clinician up to \$125 in chair side time for each procedure.

Classic Method	Minutes	Quick Up Method	Minutes
Prepare recess	10	Prepare recess	10
Prepare two vent holes	4	<i>No vent holes</i>	–
Block out attachment parts with silicone wax	8	Block out attachment parts with Fit Test	5
Apply primer	1	Apply primer	1
Apply pick-up material/reline by over filling and let it set	8	Apply pick-up material <i>under filling</i> and let it set	3.5
Remove excess material	10	Use Quick Up LC to fill gaps	3
Polish	10	Polish	3
Total Minutes	51	Total Minutes	25.5
Total Chairside Cost (\$5 per min)	\$255	Total Chairside Cost (\$5 per min)	\$128

*Example with two implant pick ups. According to the ADA the average chair time cost is \$300 per hour. Depending on the skills and the cost structure of each clinician the results can be different from this table. We recommend that you do your own calculation based on your experience and individual office costs.

Presentation

- REF 1625 Kit 7.5 g QuickMix syringe, 2 g syringe Quick Up LC, 4ml Adhesive, 5 ml QuickMix syringe Fit Test C & B, accessories
- REF 1626 7.5 g Quick Up QuickMix syringe, accessories
- REF 1627 2 g syringe Quick Up LC, accessories
- REF 1628 4 ml bottle Quick Up adhesive



VOCO America Inc.
1285 Rosemont Drive
Indian Land · SC 29707

www.vocoamerica.com
infousa@voco.com

Toll-free phone: 1-888-658-2584
Fax: 1-888-849-3989

